


Instrument Panel Compartment Housing Replacement (RHD)

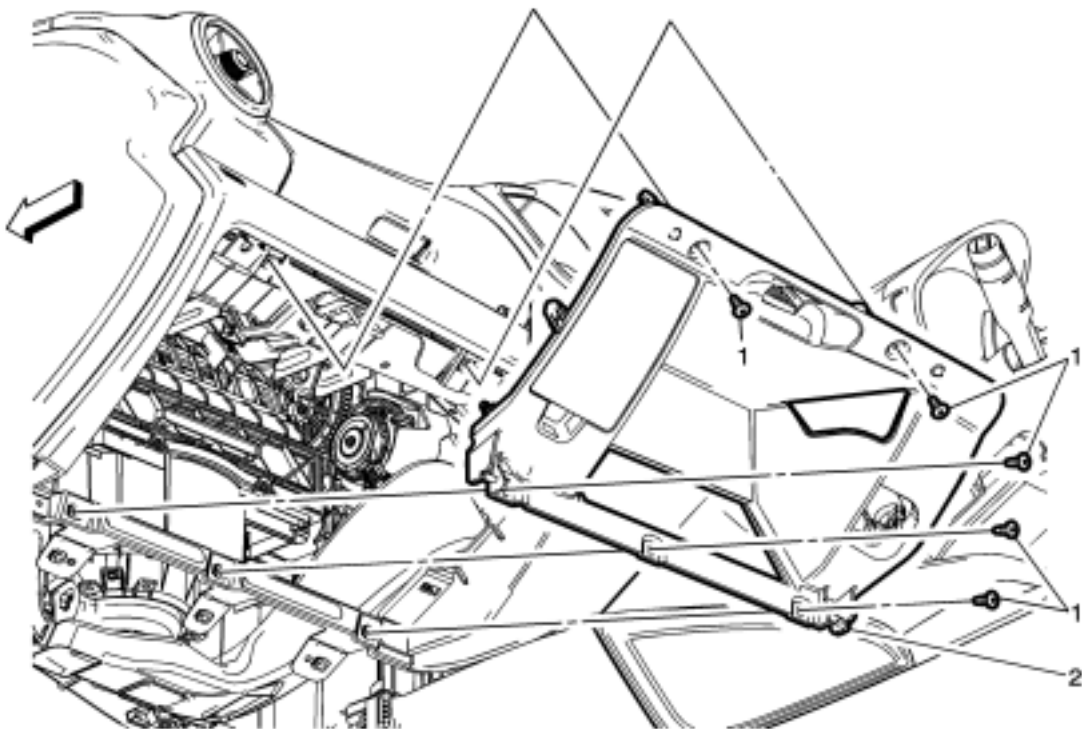

Callout	Component Name
<p>Preliminary Procedure</p> <p>Remove the instrument panel lower compartment. Refer to Instrument Panel Lower Compartment Replacement .</p>	
1	<p>Instrument Panel Compartment Housing Fastener (Qty: 5)</p> <p>Caution: Refer to Fastener Caution .</p>
2	<p>Instrument Panel Compartment Housing</p> <p>Procedure</p> <p>Grasp the housing and pull downward disengaging the retainer clips securing the housing to the instrument panel.</p>